

**Corrigendum to:
“Removing ECG Artifact from the Surface
EMG Signal Using Adaptive Subtraction
Technique” published in J Biomed Phys Eng
2014; 4(1):31-38**

Abbaspour S.^{1*}, Fallah A.¹

In the version of this article initially published, there was an error in figure 6. The corrected figure 6 was as below.
This error has been corrected in the PDF version of the article.

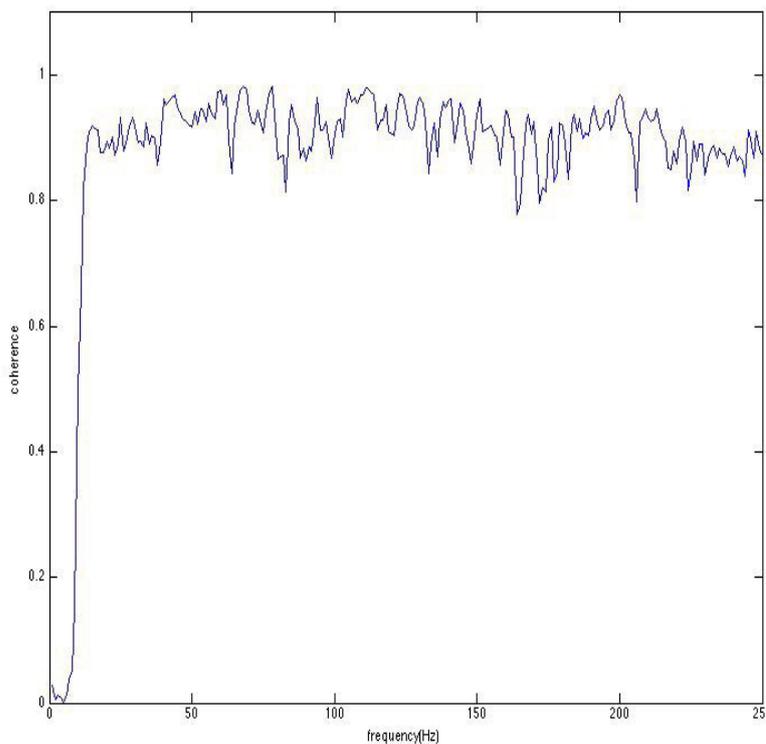


Figure 6: Coherence of clean EMG and cleaned EMG signals.

Conflict of Interest

None

¹Department of Biomedical Engineering, Amirkabir University of Technology, Tehran, Iran

*Corresponding author:
S. Abbaspour
Department of Biomedical Engineering,
Amirkabir University of Technology, 424 Hafez Ave, Tehran, Iran
E-Mail:
sara.x.abbaspour@mdh.se